


My sleep therapy:
getting started with
the AirSense™ 11 or
AirCurve™ 11 machine



Treating your sleep apnoea could improve your energy and health. When you set up a ResMed AirSense 11 or AirCurve 11 machine, you're taking an important step in the right direction.

This document explains how to use your new equipment. It is not intended to replace the manufacturer's user guide. For any additional questions relating to the use of the product, please refer to the user manual supplied with the product.

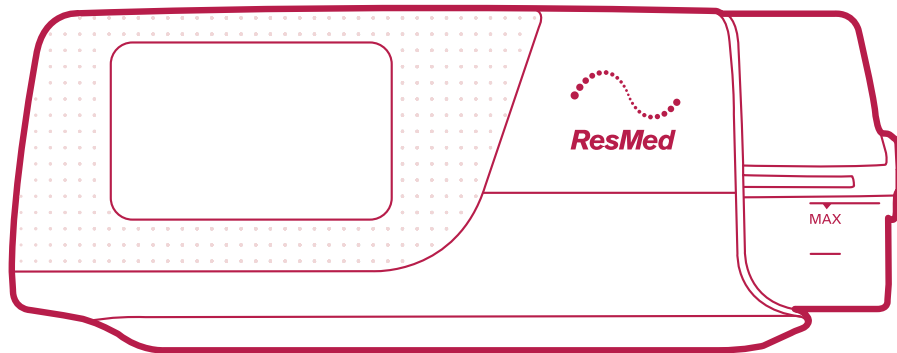

Prefer to watch a video?

Scan the QR code or visit
[ResMed.com/RemoteSetup](https://www.resmed.com/RemoteSetup)
to see the setup process in action

Benefits of sleep apnoea treatment

Finding an OSA treatment that works for you – and sticking with it – can have a real and positive impact on your day-to-day life. Here are some of the main benefits that people can experience¹ if they start – and stick with – therapy.

Fewer risks and symptoms:









- 64% reduction in risk of cardiovascular disease among patients treated with CPAP therapy compared to patients receiving no treatment at all.²
- Reduction in motor vehicle collisions. People with untreated sleep apnoea are up to 2.5 times more likely than normal sleepers to have traffic accidents.³
- Lower daytime and night-time blood pressure.⁴

Better quality of life:

- Reduced sleepiness.⁵
- Improved cognitive function.⁵
- Improved depressive symptoms in people with comorbid depression.^{6,7}

What's inside?

- A** Device travel bag
- B** Quick start guide
- C** AirSense 11 or AirCurve 11 machine
- D** HumidAir™ 11 humidifier tub*
- E** Air tubing
- F** Power supply unit and power cord
- G** User guide
- H** 2 standard filters

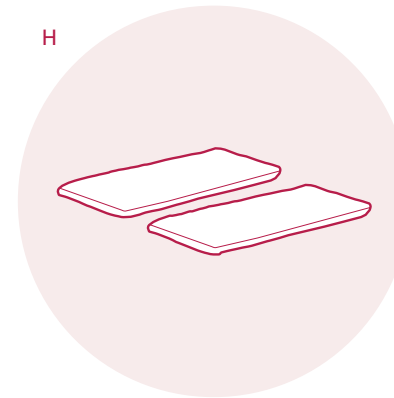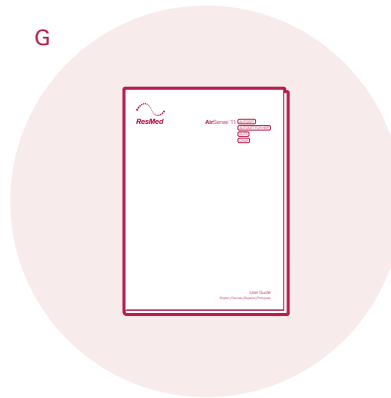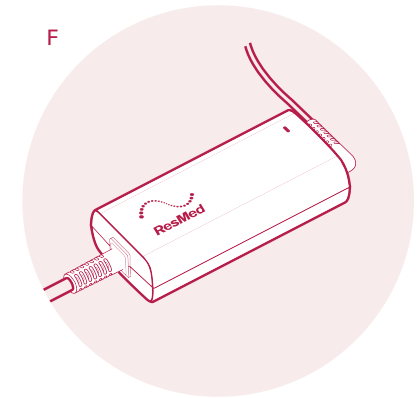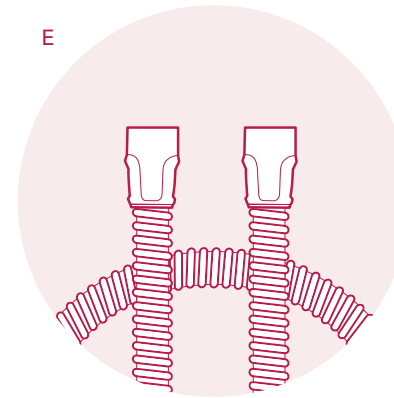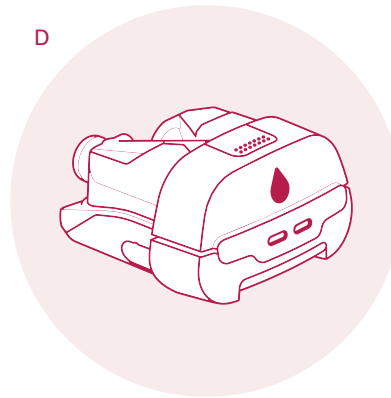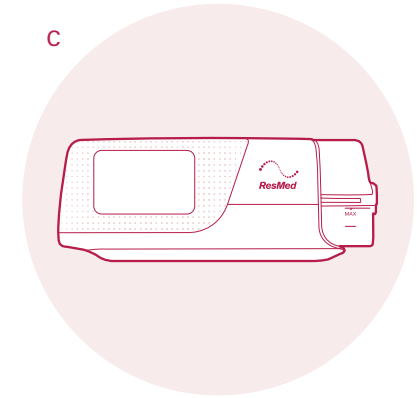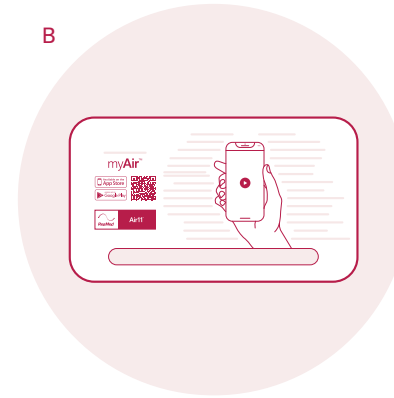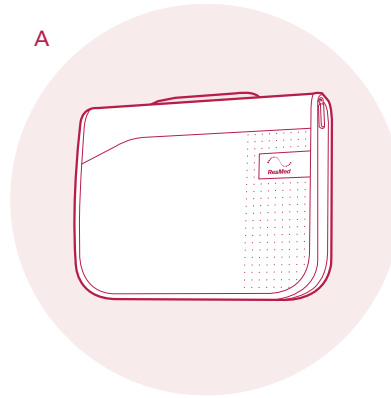




**only if you have been prescribed a humidifier with your machine.*

STEP 1

Setting up your machine

Let's begin by setting up your AirSense 11 or AirCurve 11 machine.

- A** Place the device on a stable, level surface and connect the power cord into the power inlet at the rear of the device.
- B** Connect one end of the power cord to the AC adaptor and the other end to the power outlet.
- C** Your machine will power on and display the Welcome screen. You might need to select your language. On the Welcome screen, select 'USER'.
- D** You'll be asked to answer some simple questions and will be invited to continue your setup with or without the myAir app.

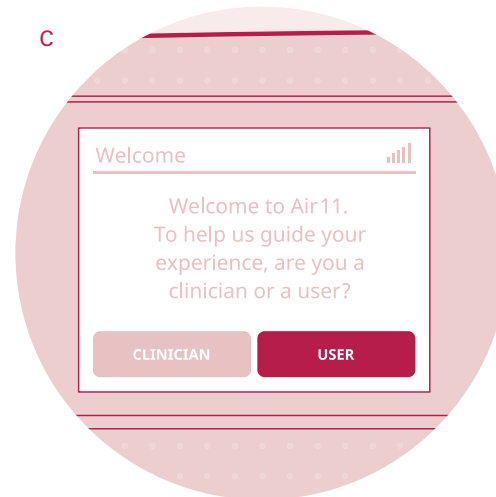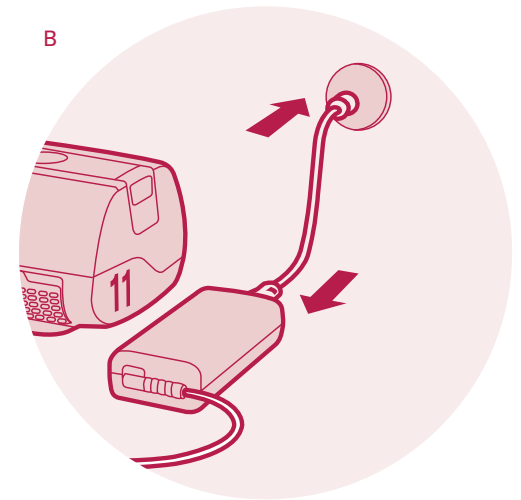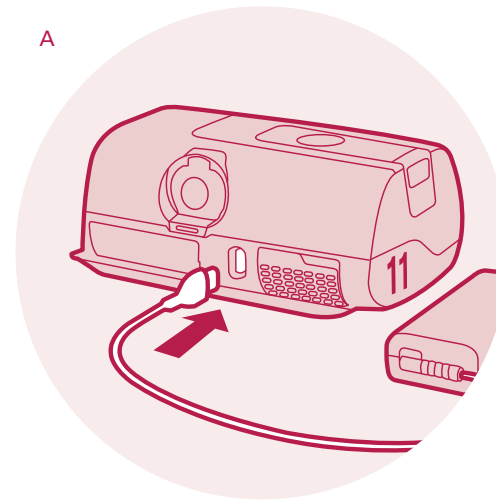


Setting up the myAir app

To make the most of your device, download the myAir app. It offers personalised support to build your skills and confidence. It guides you through device and mask setup with clear, step-by-step 'how-to' videos.




A Download the myAir™ app

Search 'myAir' in the App Store or on Google Play to download the app to your phone. You can also scan the QR code above using your smartphone camera.

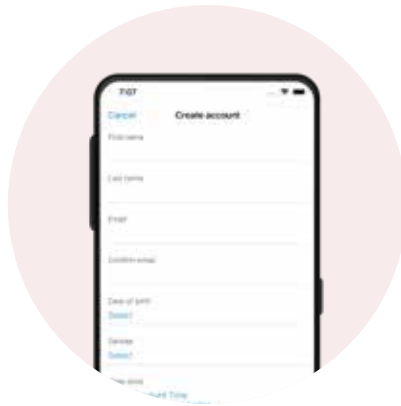

B Sign in or create account

If you already have a myAir account, you can sign in directly with your username and password. If you're a new user, click 'Create account' and fill in the required fields.

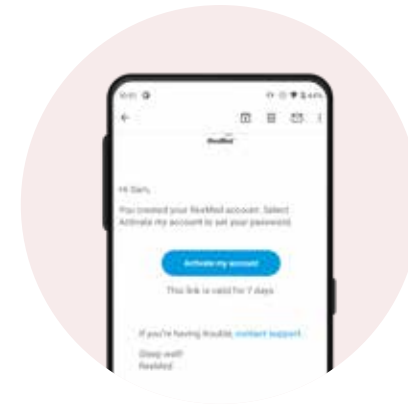

C Activate your account

Check your inbox – you should receive an email from myAir asking you to activate your account. Click on the link in the email, then follow the prompts to create your password.


If you can't see an activation email in your inbox, please check your spam folder.



D 2-Step Verification

To access myAir, you have to enter your log-in information (step 1) and then enter a one-time passcode that is sent by email (step 2).

Note: To switch off the one-time passcode option and log in directly in the future, tick 'Remember this device'.

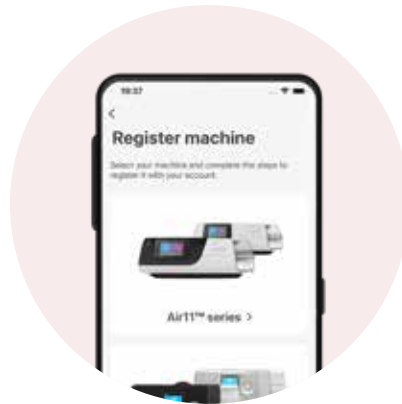

E Add your equipment

1. Add machine

Follow the instruction on your app, you will need to enter the 4-digit key displayed on the machine touchscreen to complete Bluetooth™ pairing*.

2. Add mask

Select brand and model.



F Continue the setup process


The myAir app will suggest you use the Personal Therapy Assistant feature, which will guide you through the rest of the setup process. Click on 'Get started'.

**Bluetooth must be turned on in smartphone settings*

Attaching your air tubing

Follow step-by-step instructions on the myAir app or follow the steps below:

- A** Find your air tubing in the pocket of your machine travel bag.
- B** Connect your air tubing by holding the cuff and lining it up with the connector port on the back of the machine.
- C** If you have ClimateLineAir™ tubing, be sure to line up the connector pin on the tubing cuff to the corresponding slot on the connector port.
- D** Push until the cuff clicks into place.



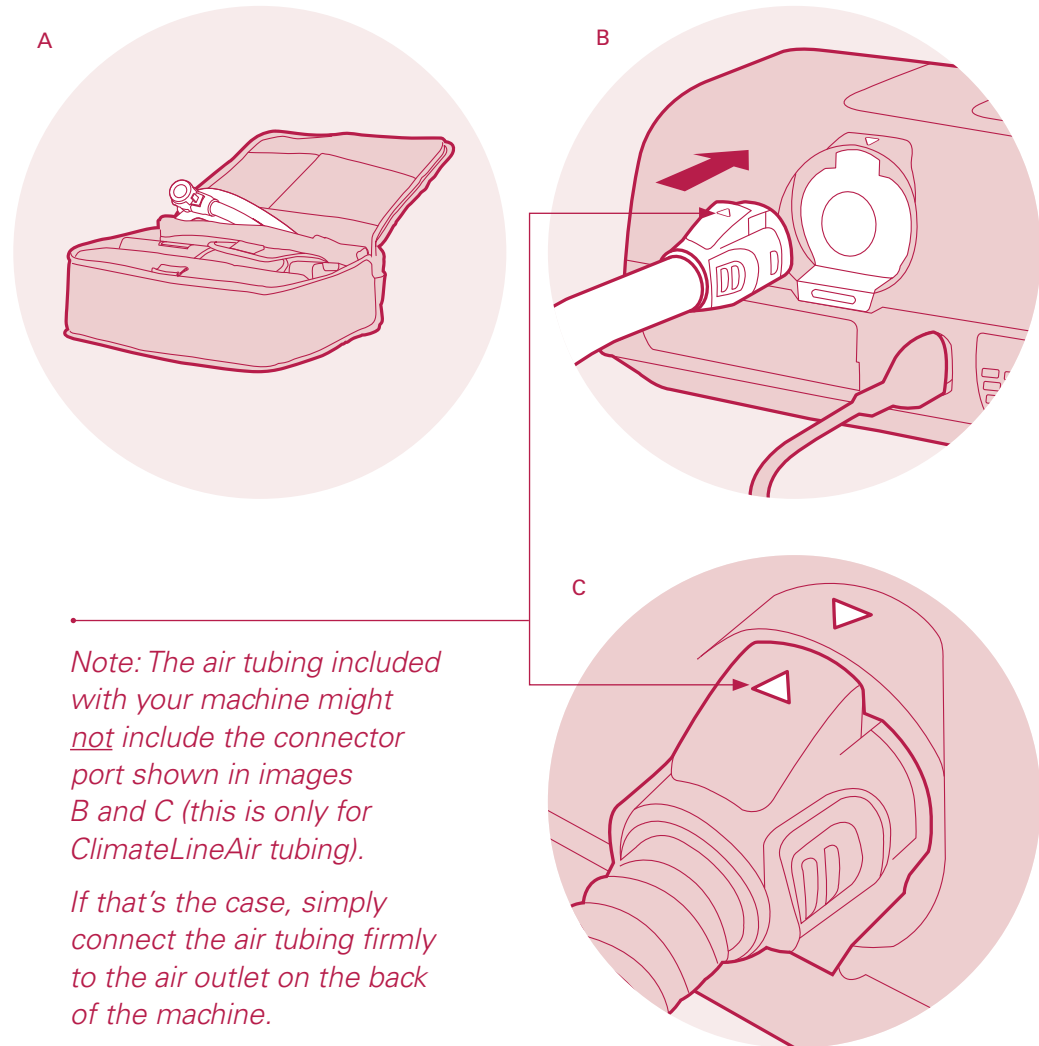


STEP 4

Preparing your HumidAir 11 humidifier tub*

Follow step-by-step instructions on the myAir app or follow the steps below:

- A** Snap open the lid of the water tub.
- B** Fill it with drinking-quality water up to the maximum water level mark.**
- C** Close the lid until it snaps shut.
- D** Gently push the water tub into the side of the machine until you feel it lock into place.

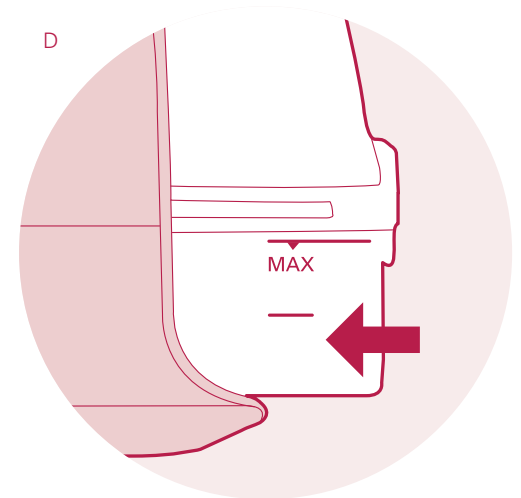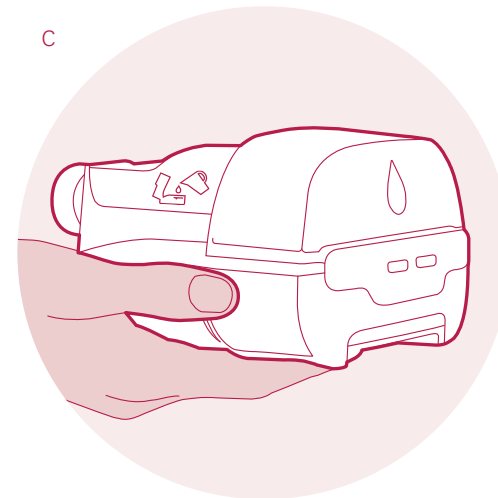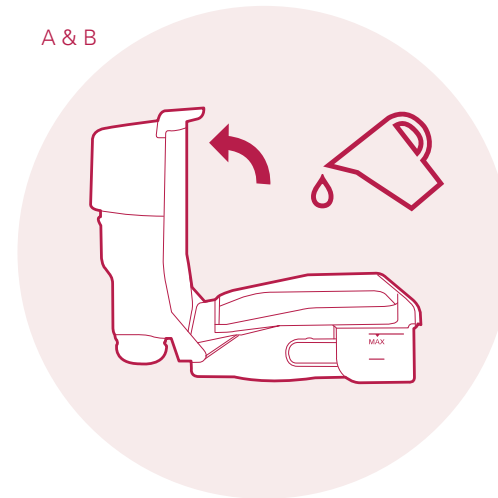

**If your machine does not have a humidifier, please do not put water in the machine.*

***Do not use any additives in the humidifier tub (eg, scented oils or perfumes).*





These may reduce humidification output and/or cause deterioration of the tub materials.

Fitting your mask




The myAir app offers step-by-step instructions to help you fit your mask and check the seal. You can also follow the steps below:

- A** With your mask on your face, connect the tube from your machine to your mask.
- B** On the Home screen, select 'More'.
- C** Under 'THERAPY', tap the Mask Fit option and select 'START'.

The machine will start blowing air and a green tick will automatically appear on the screen. Wait a few seconds while the machine checks your mask fit.

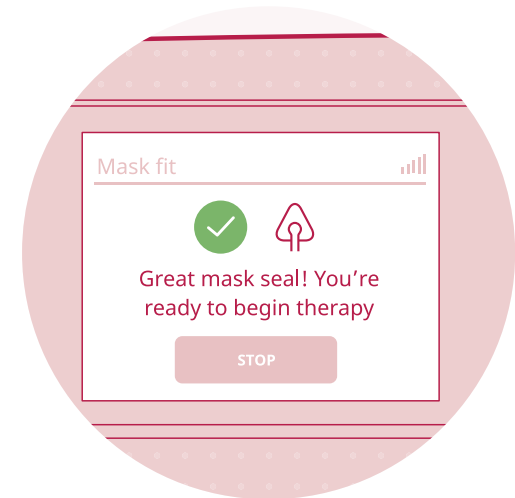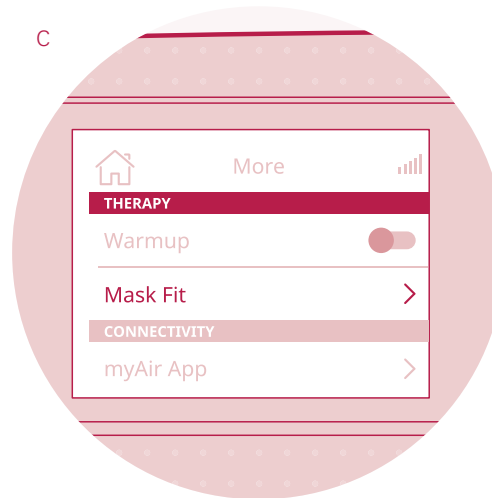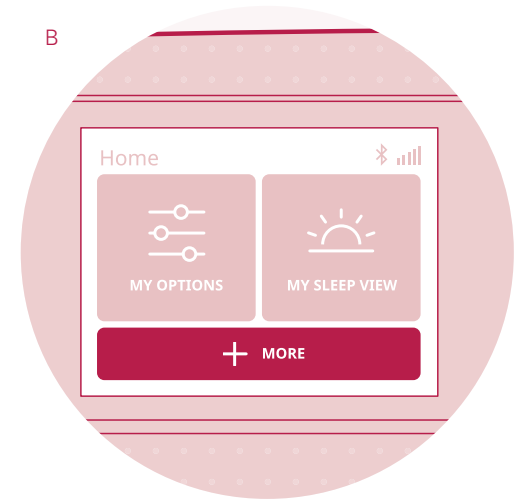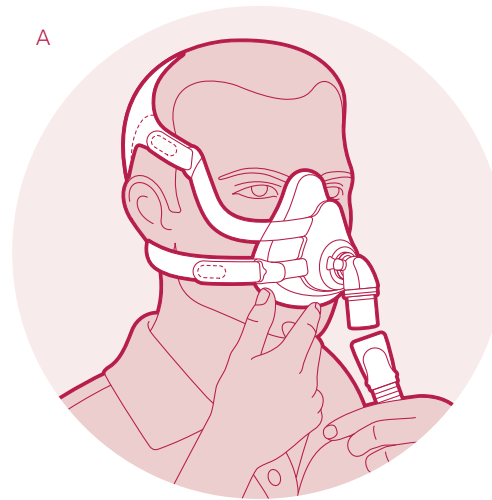


- D** If the green tick changes to an orange exclamation mark, your mask may be leaking and you might need to make small adjustments to the fit.
- E** Readjust the top and bottom headgear straps so that your mask fits snugly but is not pulled tight. You can also pull the mask away from your face and gently let it fall back against your skin.
- F** Wait a few more seconds while the machine checks your fit. When your mask is properly fitted, you'll see the green tick appear on the screen again.
- G** When you're ready to start therapy, press the START/STOP button.

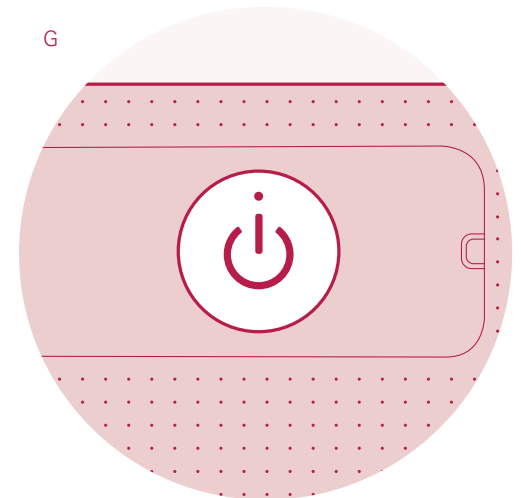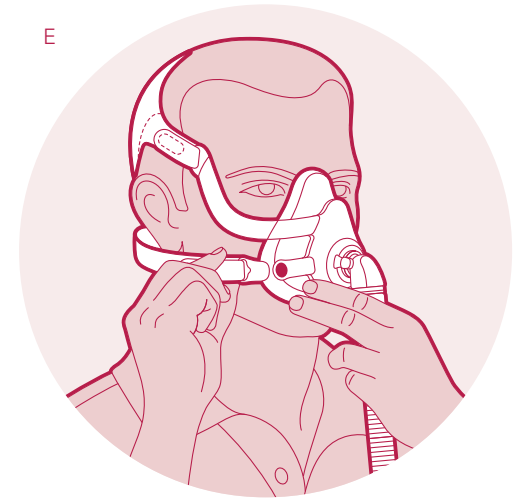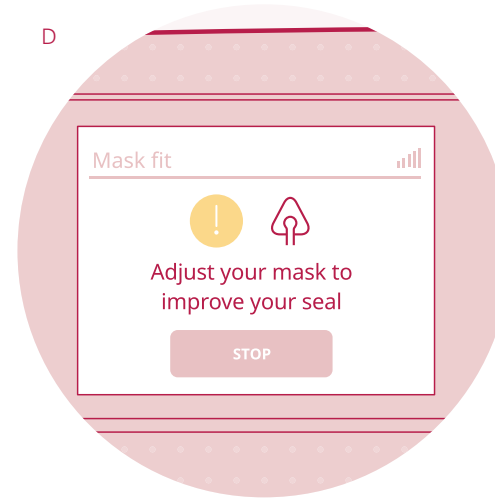

Navigating your machine


- A** The START/STOP button located on the top of your machine is used to start and stop therapy sessions.
- B** On the Home screen, tap 'MY OPTIONS' to adjust your comfort settings and tap 'MY SLEEP VIEW' to see your sleep therapy data.
- C** At any time, you can tap the 'HOME' icon in the top-left corner to return to the Home screen.

Note: You can adjust your comfort settings if you choose. All other device settings are pre-set in line with your prescription and can only be changed by a qualified healthcare professional.

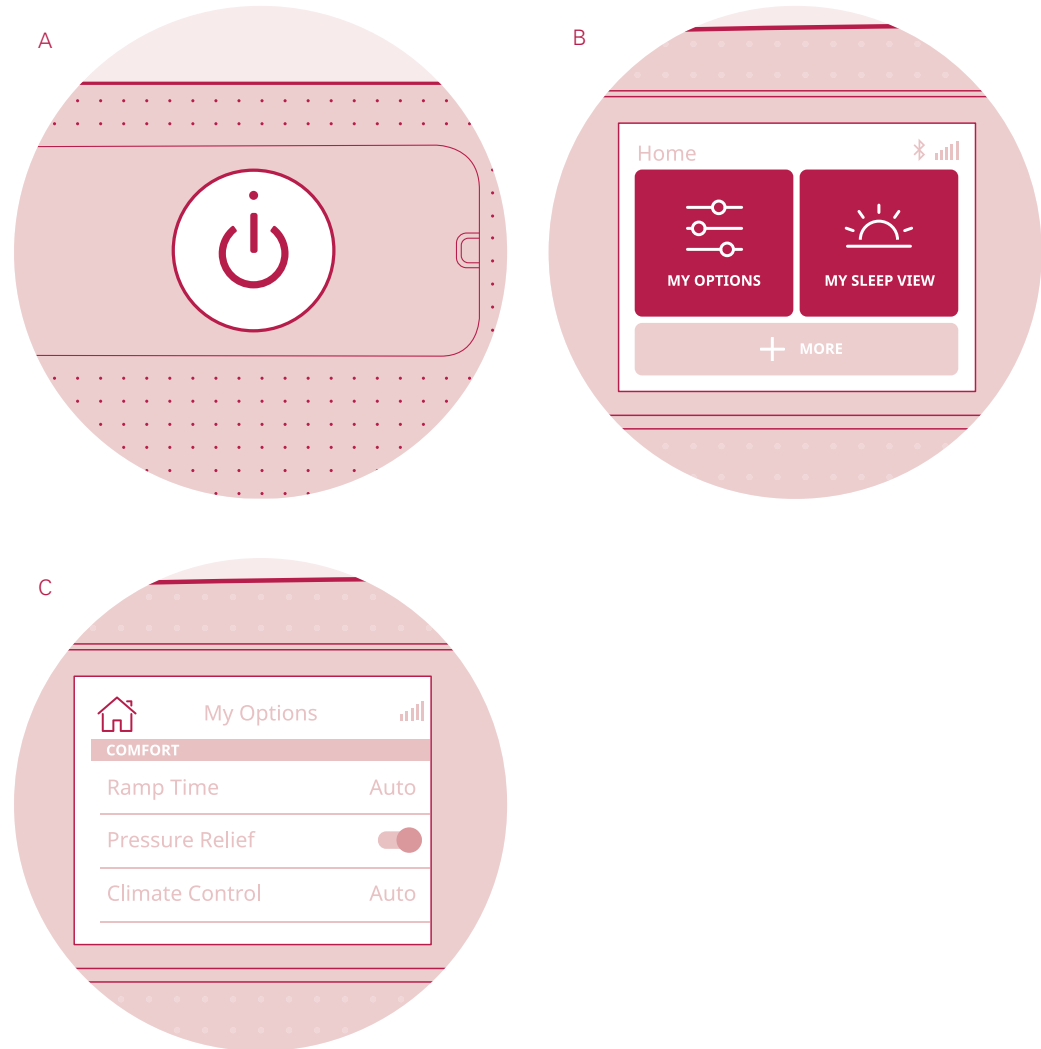

Monitoring your therapy progress with the myAir app

ResMed myAir is a free application that lets you know how you slept the night before and helps you stay on track throughout your sleep apnoea treatment journey.

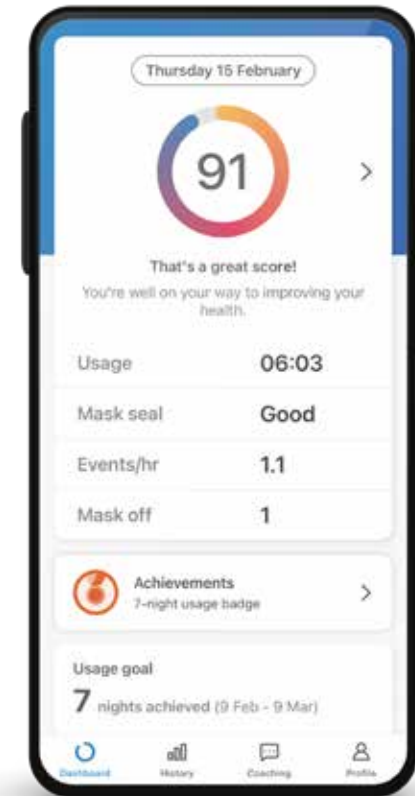

myAir score

A daily snapshot of how well you slept.

Coaching tips

Learn ways to help make your therapy more comfortable.

Alerts

Know if something is wrong with your mask or machine, and learn how to fix it.

Goal Tracking Challenge

Earn your achievement badges with goal tracking as your progress throughout your therapy and reach the '21-night' usage badge.

Personalised sleep tools

How-to instructions, videos and personalised information.

Health Trends

For a more complete picture of your therapy's impact on your overall wellbeing, you can share health app data – such as steps taken, weight and active energy – in myAir and view trends.

Care Check-In

Answer questions about your therapy and access tailored support to try to resolve minor matters independently, during the first month of therapy and then every 6 months.




Cleaning your equipment

Components should not be washed in temperatures higher than 55°C.
For cleaning your mask, refer to the mask user guide for detailed instructions.*



Prefer to watch a video?
Scan the QR code to see the process in action

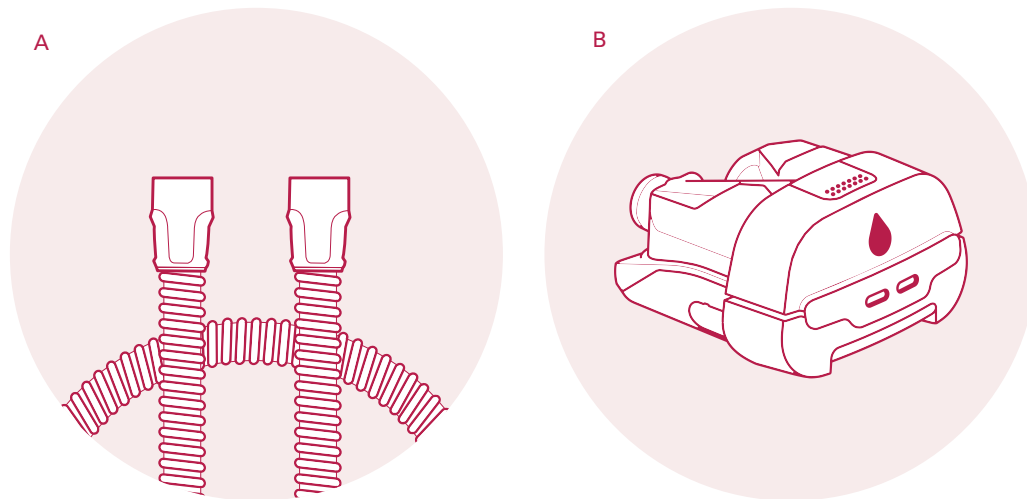

A Air tubing

Weekly cleaning

1. Wash it in warm water using a mild dishwashing liquid.
2. Rinse thoroughly in water.
3. Allow to dry out of direct sunlight or heat.

B Humidifier

Daily cleaning


1. Empty the humidifier tub and wipe it thoroughly with a clean disposable cloth. Allow it to dry out of direct sunlight.
2. Refill the humidifier tub with drinking-quality water.

Weekly cleaning

1. Wash it in warm water using a mild dishwashing liquid OR in a solution of 1 part white vinegar to 9 parts water at room temperature.
2. Rinse thoroughly in water.
3. Allow to dry out of direct sunlight or heat.
4. Wipe the exterior of the device with a dry cloth.

Note: The humidifier tub may be washed in a dishwasher.

**Beware of electrocution: Do not immerse the device, AC adaptor or power cord in water. Do not connect to power while the device is wet. Make sure that all parts are dry before plugging it in. If liquids are spilled into or onto the device, unplug the device and let the parts dry.*

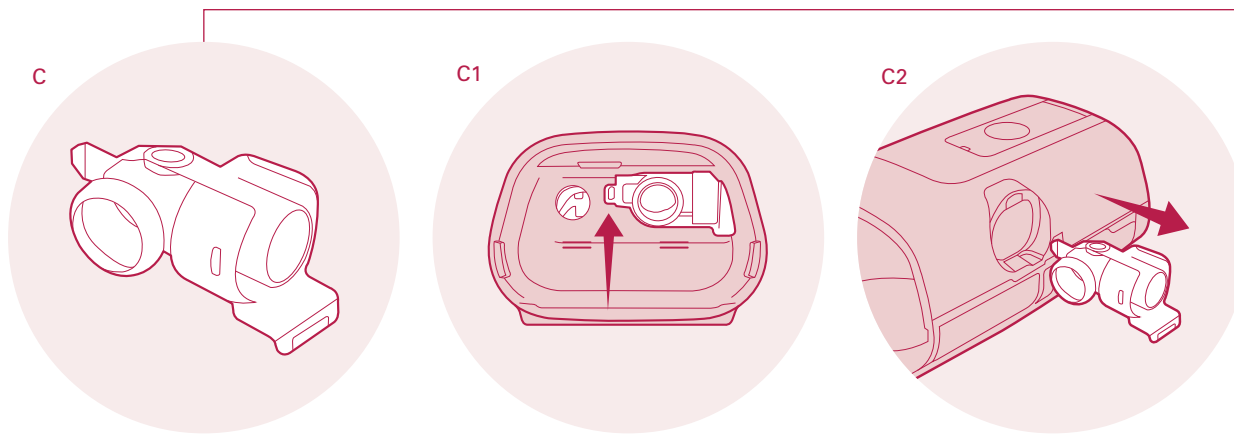

Note: The outlet connector may be washed in a dishwasher.


C Outlet connector

Disassembling the outlet connector

1. Locate the outlet connector on the inside of the device and release it by pressing the clip firmly.
2. Remove the outlet connector by pulling it out through the outlet connector socket at the rear of the device.

Weekly cleaning

1. Wash it in warm water using a mild dishwashing liquid OR in a solution of 1 part vinegar to 9 parts water at room temperature.
2. Rinse thoroughly in water.
3. Allow to dry out of direct sunlight or heat.

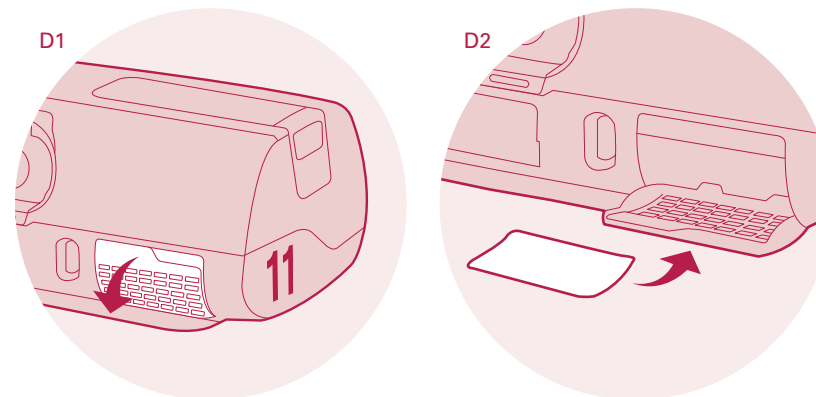

D Air filters

Replace them every 6 months

1. Open the air filter cover and remove the old air filter.
2. Place a new air filter onto the air filter cover and then close the cover. Make sure the air filter and air filter cover are fitted at all times to prevent water and dust from entering the device.

Note: The air filter is not washable or reusable.



For more information about setting up ResMed equipment, visit **ResMed.com/RemoteSetUp**

For specific questions about your equipment, contact your equipment provider or

ResMed customer support on +44 1235 862997

Please refer to the user guides for relevant information related to any contraindications, warnings and precautions to be considered before and during use of the products. ASV therapy, with AirCurve 11 ASV PaceWave, is contraindicated in patients with chronic, symptomatic heart failure (NYHA 2-4) with reduced left ventricular ejection fraction (LVEF \leq 45%) and moderate to severe predominant central sleep apnoea.

1 Epstein LJ; Kristo D; Strollo PJ; Friedman N; Malhotra A; Patil SP; Ramar K; Rogers R; Schwab RJ; Weaver EM; Weinstein MD. Clinical guideline for the evaluation, management and long-term care of obstructive sleep apnea in adults. *J Clin Sleep Med* 2009;5(3):263-276.

2 Buchner NJ et al. Continuous positive airway pressure treatment of mild to moderate obstructive sleep apnea reduces cardiovascular risk. *Am J Respir Crit Care Med*. 2007;176(12):1274-1280.

3 Bonsignore, M.R., et al., European Respiratory Society statement on sleep apnoea, sleepiness and driving risk. *Am J Respir Crit Care Med*, 2021. 57(2).

4 Fava C, Dorigoni S, Dalle Vedove F, et al. Effect of CPAP on blood pressure in patients with OSA/hypopnea: a systematic review and meta-analysis. *Chest*. 2014;145(4):762-771.

5 Sánchez AI, Martínez P, Miró E, Bardwell WA, Buela-Casal G. CPAP and behavioral therapies in patients with obstructive sleep apnea: effects on daytime sleepiness, mood, and cognitive function. *Sleep Med Rev*. 2009;13(3):223-233.

6 Povitz M, Bolo CE, Heitman SJ, Tsai WH, Wang J, James MT. Effect of treatment of obstructive sleep apnea on depressive symptoms: systematic review and meta-analysis. *PLoS Med*. 2014;11(11):e1001762.

7 Wiggins, A.J., et al., Continuous positive airway pressure versus standard care for the treatment of people with mild obstructive sleep apnoea (MERGE): a multicentre, randomised controlled trial. *Lancet Respir Med*, 2019.