

Autof ms1000

MALDI-TOF

Automated Mass
Spectrometry Microbial
Identification System



Autobio
Autof
MS1000



AUTOMATED MASS SPECTROMETRY MICROBIAL IDENTIFICATION SYSTEM

Hardy Diagnostics is proud to introduce the Autof ms1000*

Identification of microorganisms to the species level is the principle **objective** in microbiology.¹ For many years, such a feat has been accomplished through laborious biochemical assays. While advancements in nucleic acid sequencing technologies have enabled highly specific detection rates of microorganisms, these technologies are too **time-consuming** and **costly** to be commonplace.²

The **Autof ms1000** provides **automated, high-speed** and high-confidence identification and taxonomical classification of bacteria, yeasts, and fungi based on proteomic profiling. Numerous studies have demonstrated the **higher accuracy, faster time-to-result**, and lower cost provided by MALDI-TOF technology when compared to classical methods.^{3,4,5}

Features:

- Faster time-to-result when compared to conventional methods and PCR⁶
- Accuracy similar to nucleic acid sequencing technologies⁷
- Cost effective⁸
- Robust, intuitive software, supporting 21 CFR part 11 compliance
- Installation Qualification/Operation Qualification/Performance Qualification support
- LIMS/LIS connectivity and support
- Database of approximately 5,000 species created with over 17,000 strains
- Can identify 96 samples in less than 20 minutes hands-on time



Cat. no. MS1000

1. <https://www.ncbi.nlm.nih.gov/books/NBK8406/> 2. <https://pubmed.ncbi.nlm.nih.gov/24822116/>

3. <https://www.ncbi.nlm.nih.gov/pmc/articles/PMC5986882/> 4. <https://pubmed.ncbi.nlm.nih.gov/31116624/>


5. <https://www.ncbi.nlm.nih.gov/pmc/articles/PMC5228263/> 6. <https://pubmed.ncbi.nlm.nih.gov/31116624/>

7. <https://www.ncbi.nlm.nih.gov/pmc/articles/PMC5986882/> 8. <https://www.ncbi.nlm.nih.gov/pmc/articles/PMC5228263/>

INTUITIVE SOFTWARE

Easy-to-use software provides a friendly user experience. The Autof Acquirer has been designed to comply with the rigors and standards of a regulated working environment.




- Authentication
- User management
- Data archiving

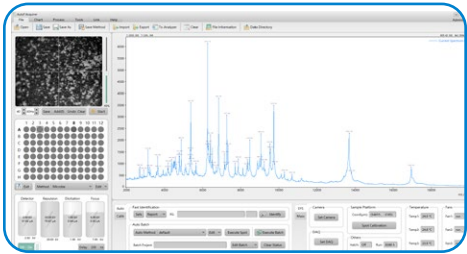

Range	Description	Color
9.500 - 10.000	Reliable species	Green
9.000 - 9.499	Reliable species identification result	Green
6.000 - 8.999	Reliable genus identification result	Yellow
0.000 - 5.999	No reliable identification result	Red

Easy-to-read, color coded score annotations indicate the degree of confidence in each identification result.

Following the acquisition of spectral profiles, an identification report is automatically generated. A summary of sample names, descriptions, identification results, and scores will be displayed.

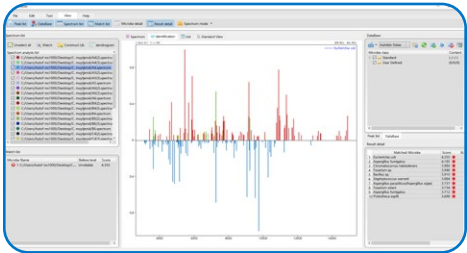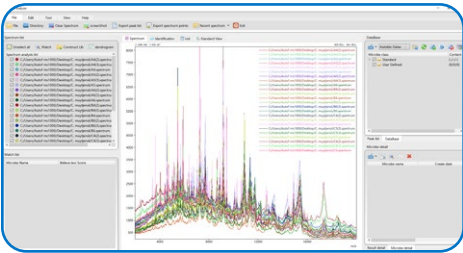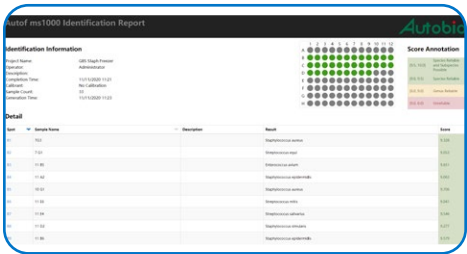


Laboratories that need to create their own local database can do so with the included companion software application, Autof Analyzer.

THE PROCESS

SINGLE COLONY


SINGLE SPOT

SINGLE DROP

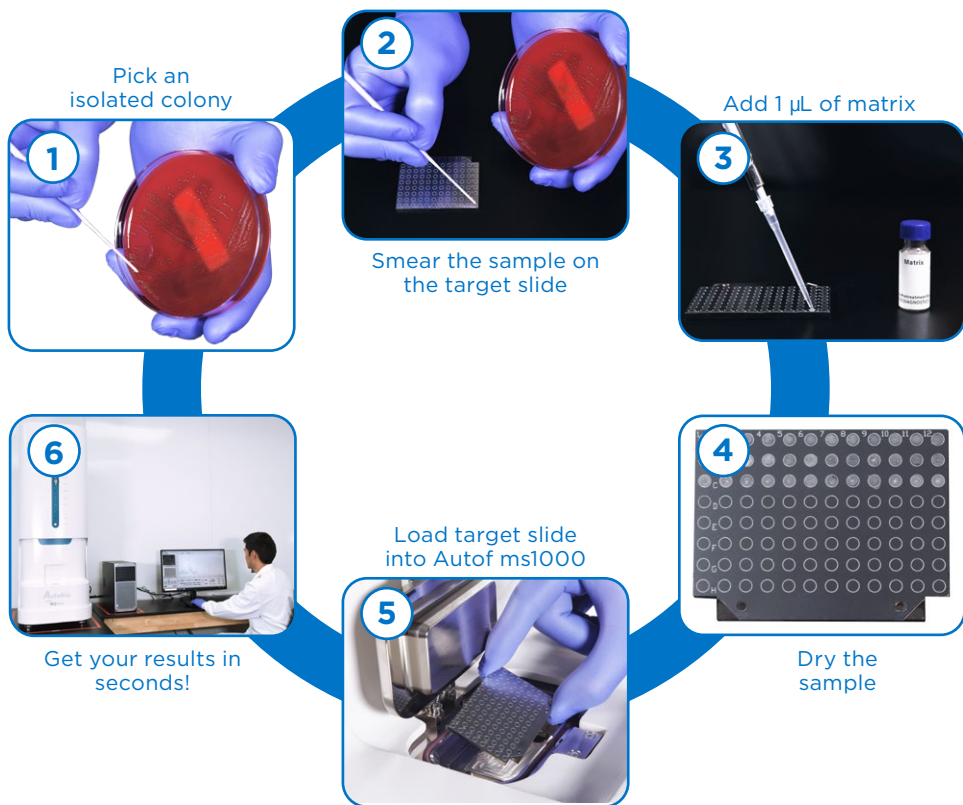

- Unique rapid identification function displays a test result in 0.1 seconds for a single sample
- Average identification (acquisition and data analysis) time for 96 samples is 17.5 minutes
- Batch function available to edit and identify samples in a fully customizable format
- Access to LIMS/LIS system; reports release automatically

FREE ASSISTANCE WITH QUALIFICATION OF THE AUTOF MS1000



The qualification process-implementation and validation of the Autof ms1000 is supported by Installation Qualification (IQ) and Operational Qualification/Performance Qualification (OQ-PQ) documentation, which is provided at no charge.

IQ

OQ-PQ

Autof ms1000 software suite is 21 CFR part 11 compliant and offers complete workflow traceability.


IQ: Verification process that ensures the Autof ms1000 has been properly delivered and installed by way of an approved system and specification checklist.

OQ-PQ: A collection of test cases employed to verify that the Autof ms1000 and its subsystems perform as expected as defined by the functional requirements specifications.

ROBUST DATABASE

The Autof ms1000 has the **most expansive database** in the industry. Created with more than **17,000 strains**, many with more than **5 reference spectra**, averaging more than **10 strains per species**, the database of the Autof ms1000 provides **highly accurate results**.


Local database includes a total of
5,041 Species, and **17,662 Strains**



Gram +



Gram -



Yeast



Filamentous Fungi




Mycobacteria

As part of the partnership, **Hardy Diagnostics** and **Autobio Diagnostics Co. LTD.** are constantly **augmenting** the **Autof ms1000 database**. New strains and species are constantly being added, **improving** upon the **reliability** and **accuracy** of the system.


The **Autof ms1000** database contains a multitude of reference strains from:

- Varying geographic regions of the world
- Different specimen types
- Different culture media types
- Different growth conditions

Criteria that captures the natural phylogenetic diversity within a species.

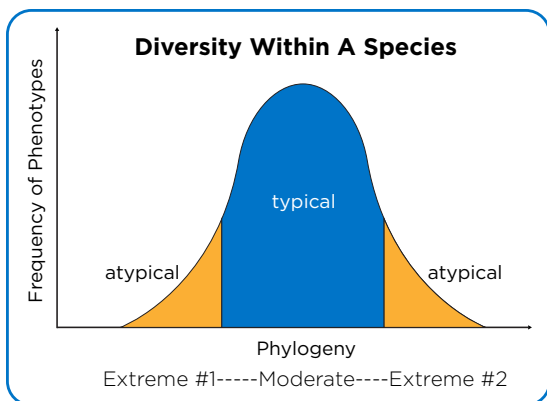


Hardy Diagnostics offers a comprehensive solution to your microbiology needs.



Culture



Identification



**Antimicrobial
Susceptibility Testing
(AST)**



40 MORE THAN Years of
Bringing You
A Culture of Service

100%
Employee Owned

ESTABLISHED
1980

MADE IN
USA

 Hardy Diagnostics
donates 1% of net
profits to charity.

 **bsi**
ISO 13485
Quality
Management for
Medical Devices
CERTIFIED

FM 572526

Hardy Diagnostics has a Quality
Management System that is certified
to ISO 13485 and is a FDA licensed
medical device manufacturer.

Headquarters

1430 West McCoy Lane
Santa Maria, CA 93455
800.266.2222
Sales@HardyDiagnostics.com
HardyDiagnostics.com

Distribution Centers

Santa Maria, California
Olympia, Washington
Salt Lake City, Utah
Phoenix, Arizona
Dallas, Texas
Des Moines, Iowa
Springboro, Ohio
Lake City, Florida
Albany, New York
Raleigh, North Carolina



For Research Use Only. Not for use
in clinical diagnostic procedures.